



# MS INSTRUMENTATION I

Vladimír Vrkoslav  
MS Group

Institute of Organic Chemistry and Biochemistry  
AS CR, v.v.i.



# MASS SPECTROMETER

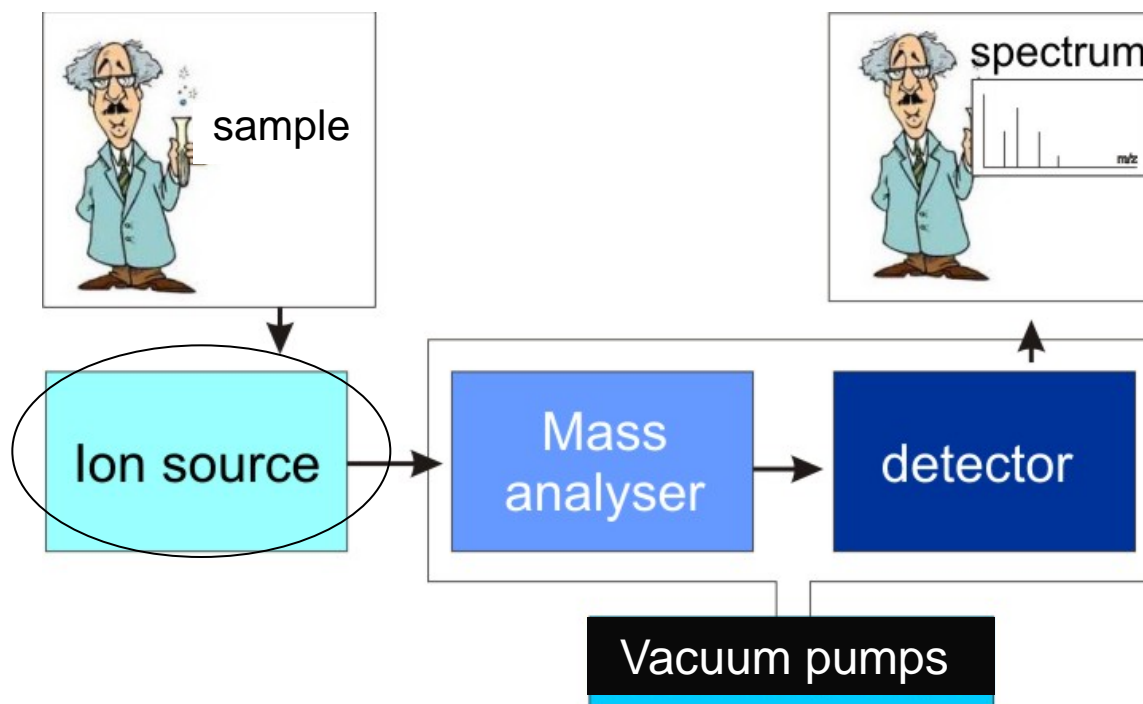

- Ion source - devices which produce positive or negative electrically charged molecules in gas phase
- Mass analysers - separate the ions according to their mass-to-charge ratio ( $m/z$ )
- Detectors - record the charge induced or the current produced, when an ion passes by or hits a surface



# ION SOURCE

Produce **positive** or negative electrically charged molecules in **gas phase**

- Choice depends on compound
  - Universal ionization technique does not exist
- Differentiation
  - By energy
    - Hard (EI)
      - Cation radical with high energy - fragmentation in ion source – many fragments in the spectra
    - Soft (CI, ESI, APCI, MALDI,...)
      - molecular adduct with low energy – no or a few fragments in the spectra
  - By pressure
    - Vacuum (EI, CI, MALDI,...)
    - Atmospheric pressure (ESI, APCI, APPI, AP MALDI,...)
- Ions
  - $M + e^- \rightarrow M^{+\cdot} + 2 e^-$  Cation radicals
  - $M + HA \rightarrow [M+H]^+ + A^-$  Molecular adducts
  - $M + B^- \rightarrow [M-H]^- + HB$  Deprotonated molecules




# DIFFERENT IONIZATION TECHNIQUE

## ○ **Molecular Analysis**

- **Electron Ionization (EI)**
- **Chemical Ionization (CI)**
- **Electrospray (ESI)**
  - **Nanoelektrospray (nanoESI)**
- **Atmospheric Pressure Chemical Ionization (APCI)**
- **Atmospheric Pressure Photoionization (APPI)**
- **Matrix-Assisted Laser Desorption/Ionization (MALDI)**
- **Laser Desorption Ionization (LDI)**
- **Secondary Ion Mass Spectrometry (SIMS)**
- **Fast Atom Bombardment (FAB)**
- **Desorption Electrospray Ionization (DESI)**
- **Desorption Atmospheric Pressure Chemical ionization (DAPCI)**
- **Direct Analysis in Real Time (DART)**
- **Thermospray (TSI)**
- .....
- .....




# ELECTRON IONIZATION (EI)

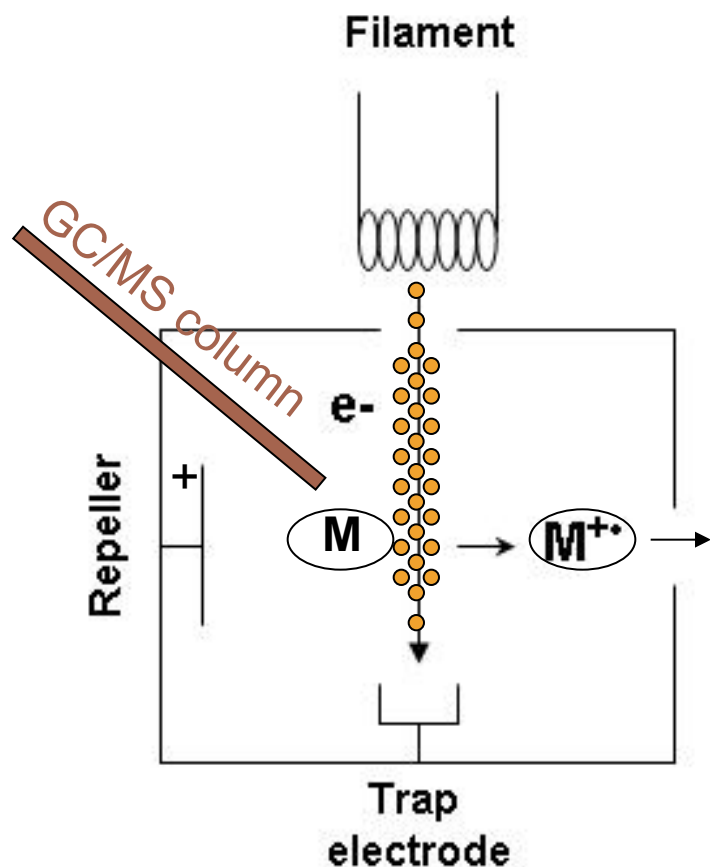

- An ionization method in which energetic electrons interact with gas phase molecules to produce ions.
  - Electron emission by heating a tungsten wire filament
  - Good reproducibility – spectral library – easy interpretation
    - (energy of the electrons 70eV)
- $M + e^- \rightarrow M^{+\bullet} + 2 e^-$ 
  - $M$  is the analyte molecule being ionized
  - $e^-$  is the electron and
  - $M^{+\bullet}$  is the resulting ion
- Widely used for volatile organic molecules
- Often coupled with GC = GC/EI-MS

# CHEMICAL IONIZATION (CI)

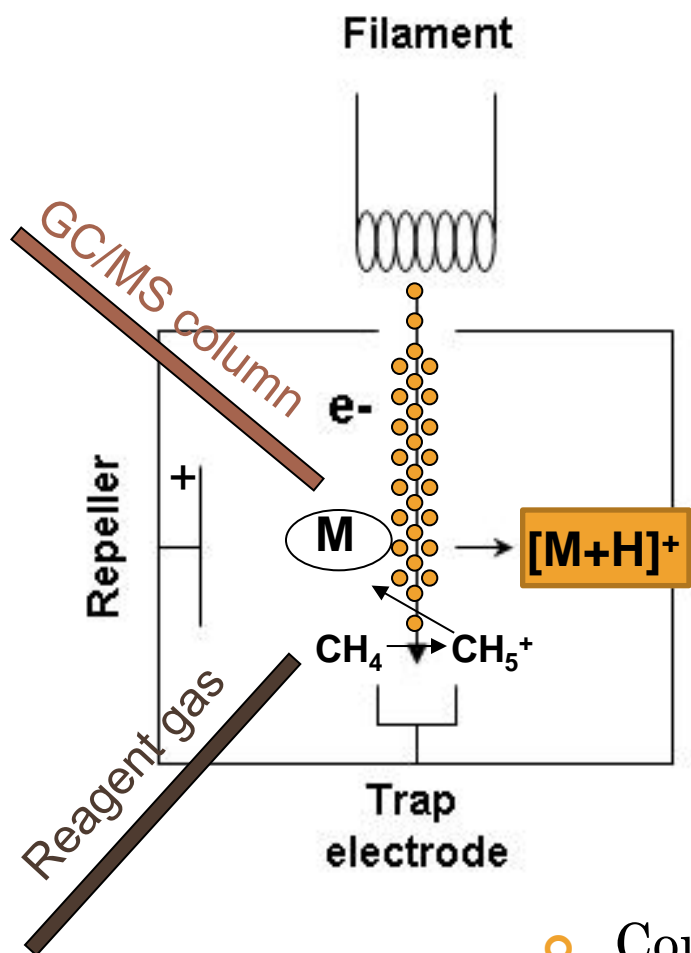

- Analyzed ions are produced through the collision of the analyte with ions of a reagent gas, that are present in the ion source

- Methane**, ammonia, isobutane, acetonitrile,.....


- Soft ionization technique

- $[M+H]^+$ ,  $[M+\text{reagent gas}]^+$ , fragments (depend on condition)



- Example

- $\text{CH}_4$  as a reagent gas




Primary ion formation



Secondary reagent ions



Product ion formation




- Coupled with GC = GC/CI-MS
- Used for volatile organic molecules




# ELECTROSPRAY (ESI)


- The liquid containing the analyte(s) is dispersed by electro spray into an aerosol
  - Charged droplets
  - Solvent evaporation
  - Coulombic explosion
- Soft ionization technique
  - $[M+H]^+$ ,  $[M+Na]^+$ ,  $[M+K]^+$ , ..... molecular adducts

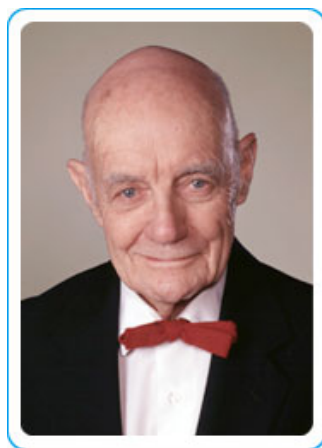

John B. Fenn  
Nobel prize in Chemistry  
2002

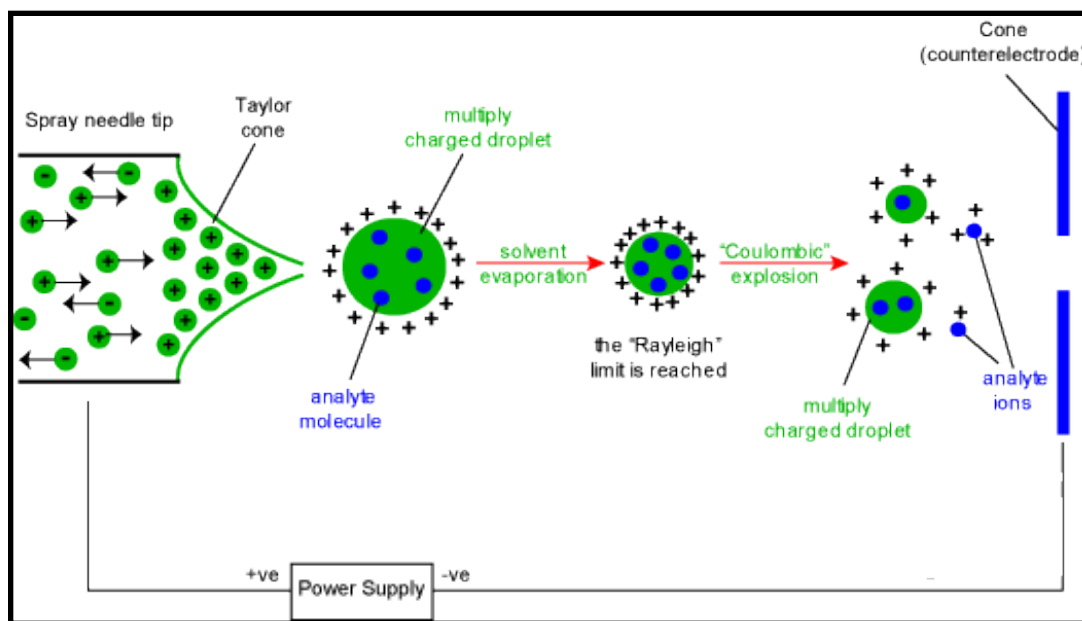

# NANOELECTROSPRAY (NANOESI)

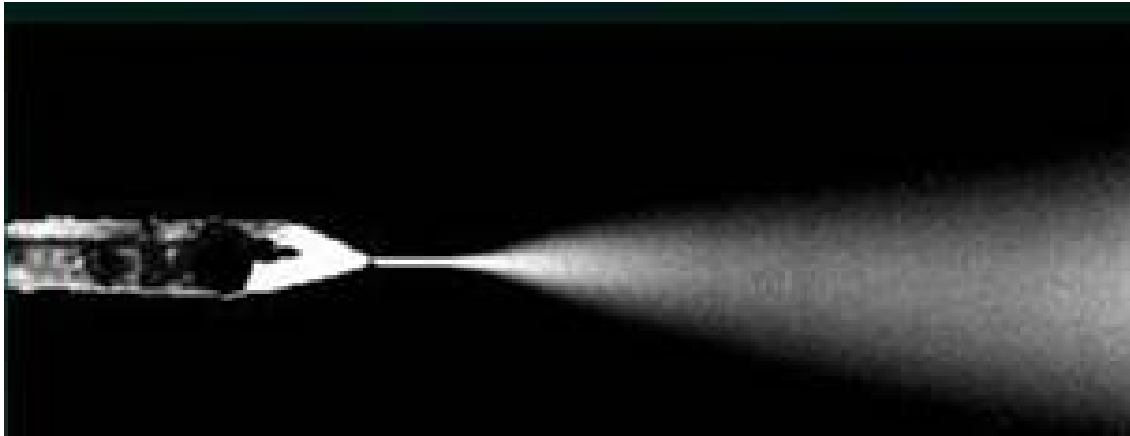

- Flow of mobile phase usually hundreds nl/min
  - ~~$[M+H]^+$ ,  $[M+Na]^+$ ,  $[M+K]^+$ , .....~~
  - Easier interpretation of the spectra

## Electrospray technique

- Polar analytes in broad mass range
- Obtaining more charged ions
  - Analysis of molecules with  $M_r$  behind the range of analyser
- Coupled with HPLC or UHPLC
  - Polar solvent (mobile phase) as a donor of  $H^+$






# ATMOSPHERIC PRESSURE CHEMICAL IONIZATION (APCI)

- The mobile phase containing eluting analyte is heated to high temperature (above 400°C), sprayed with high flow rates of nitrogen
- Molecules of solvent and gas are ionized by corona discharge
- Analyte are ionized by ionized solvent and gas molecules

## ATMOSPHERIC PRESSURE

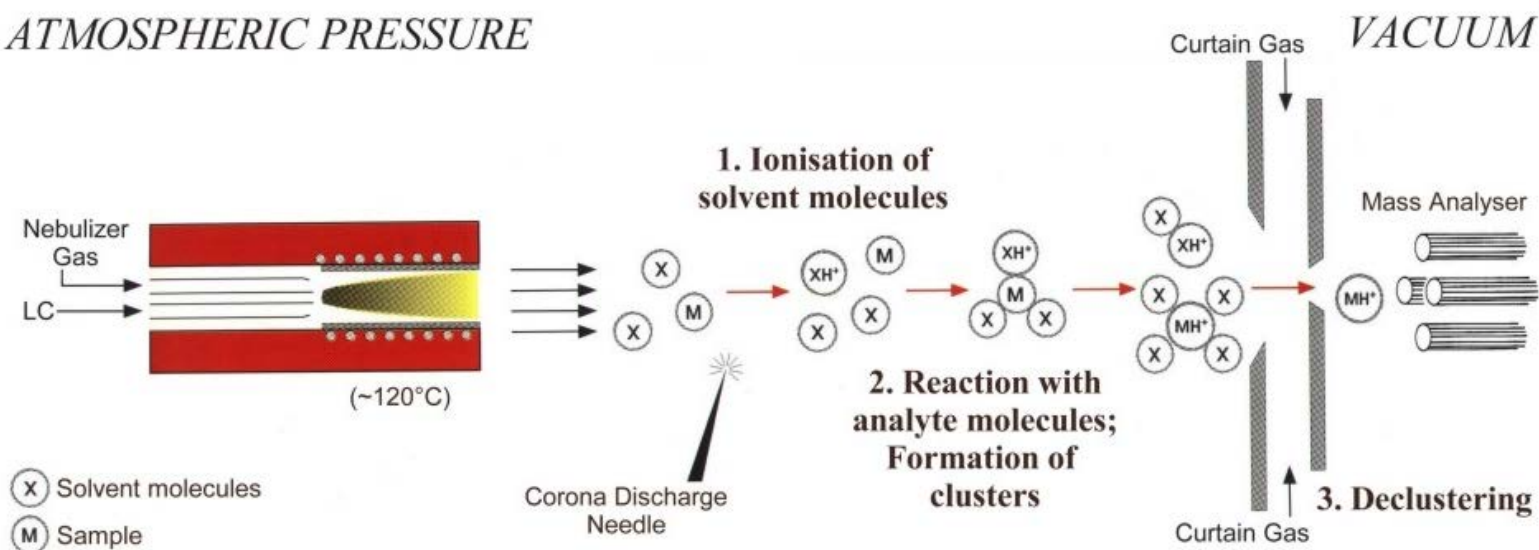


# ATMOSPHERIC PRESSURE CHEMICAL IONIZATION (APCI)

- APCI can be performed in a modified ESI source
  - Device similar to ESI source
  - However, mechanism of ionization similar to CI
- The ionization occurs in the gas phase
- APCI is a less "soft" ionization technique than ESI
  - Generates more fragment ions
- Coupled with HPLC or UHPLC
  - Advantage of APCI - it is possible to use a nonpolar solvent (mobile phase )




# MATRIX-ASSISTED LASER DESORPTION/IONIZATION (MALDI)

- Laser-based soft ionization method
  - Matrix and analyte are mixed on the target plate
  - The laser (UV, IR) shoots the mixture
  - The energy is transferred to the matrix, which is vaporized, carrying analyte into the vapour phase and charging it
- The mechanism of MALDI is still debated

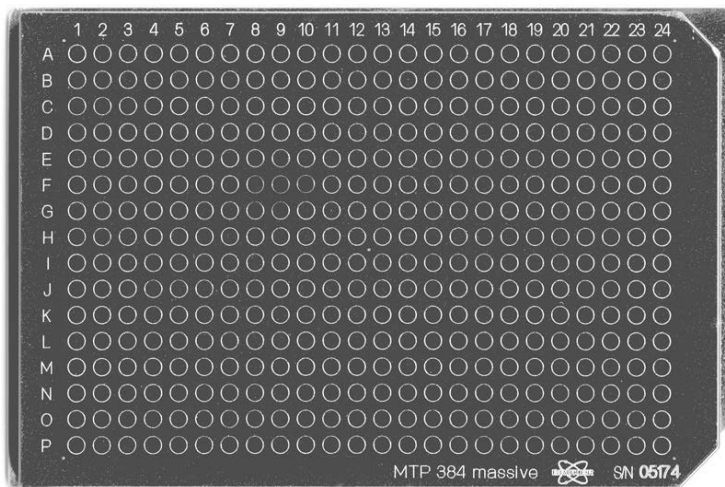

[www.ms-textbook.com](http://www.ms-textbook.com)

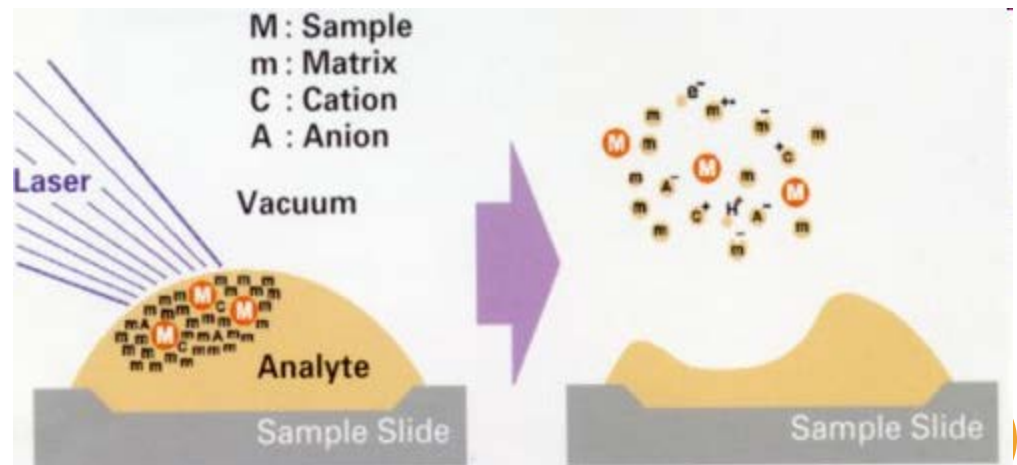

<http://www.fasmatech.net/content-61-2.html>

# MATRIX-ASSISTED LASER DESORPTION/IONIZATION (MALDI)

- Analysis of
  - Biomolecules (DNA, proteins, peptides and sugars)
  - Large organic molecules (polymers, dendrimers,...)
    - Which tend to fragment, when are ionized by more conventional ionization methods.
  - Singly charged molecular adduct
    - Molecular adducts (  $[M+H]^+$ ,  $[2M+H]^+$ ,  $[M+2H]^{2+}$ ) or loss of proton  $[M-H]^-$
    - Other molecular adducts  $[M+metal]^+$  with salts in sample (Na, K, ....., )

Franz Hillenkamp



Koichi Tanaka






Nobel prize in Chemistry 2002





# MALDI MATRICES: PROPERTIES AND REQUIREMENTS


- Small molecules, usually small organic acids
  - 2,5-dihydroxybenzoic acid, sinapic acid,  $\alpha$ -cyano-4-hydroxycinnamic acid,.....
- The MALDI matrix of requirements
  - Be able to embed analytes (by co-crystallization)
  - Be soluble in solvents compatible with analyte
  - Be vacuum stable
  - Absorb the laser wavelength
  - Cause co-desorption of the analyte upon laser irradiation
  - Promote analyte ionization




# MALDI IMAGING

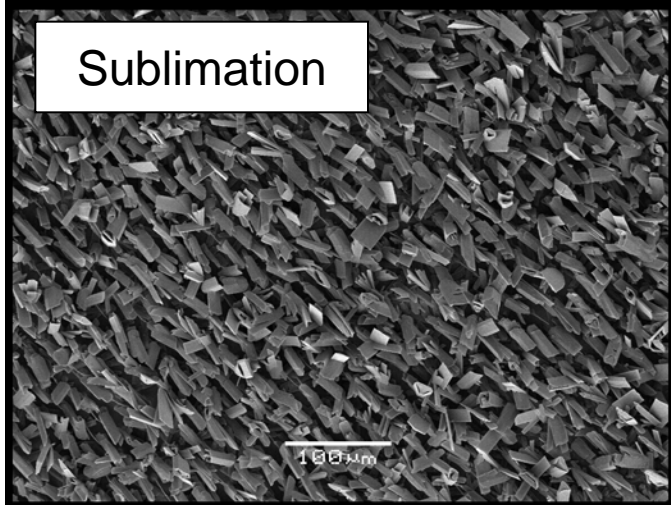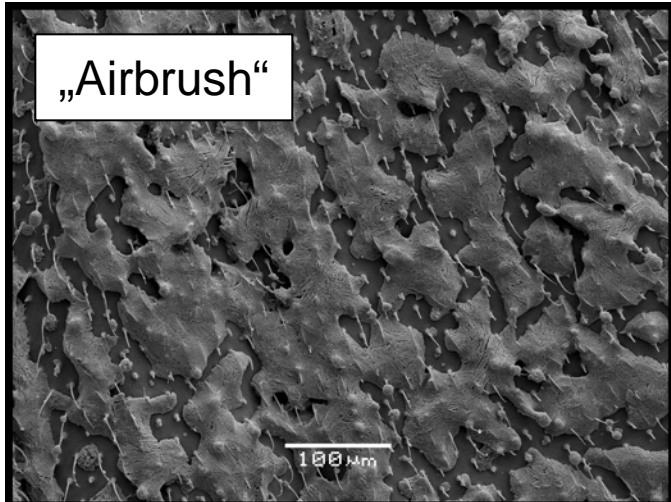


*D. melanogaster*

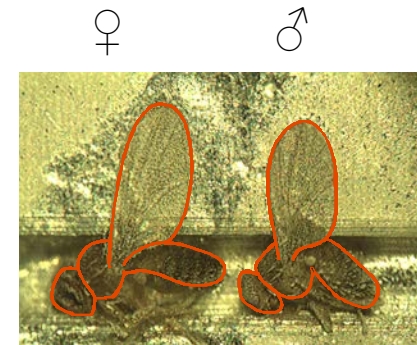

Foto

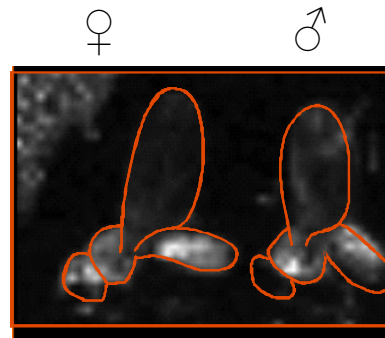

TIC

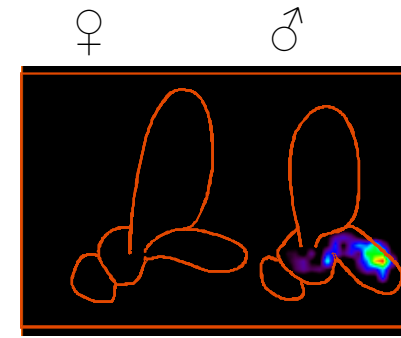

cis-vaccenyl acetate




# LASER DESORPTION/IONIZATION (LDI)

- **LDI** (laser desorption/ionization)
  - Energy of laser is directly absorbed by analyte
  - Without matrix
  - For small molecules only
    - Spectra without matrix ions
    - Better reproducibility than MALDI
    - Harder ionization technique than MALDI – fragments in spectra
    - **Sensitivity depends on analyte**
  - **Useful for imaging**
  - **Instrumentation is same as for MALDI**




# CHOICE OF IONIZATION TECHNIQUE

- Almost all compounds can be ionized by more than one technique
  - Depends on **molecular mass, polarity, ionization energy**, solubility, ...

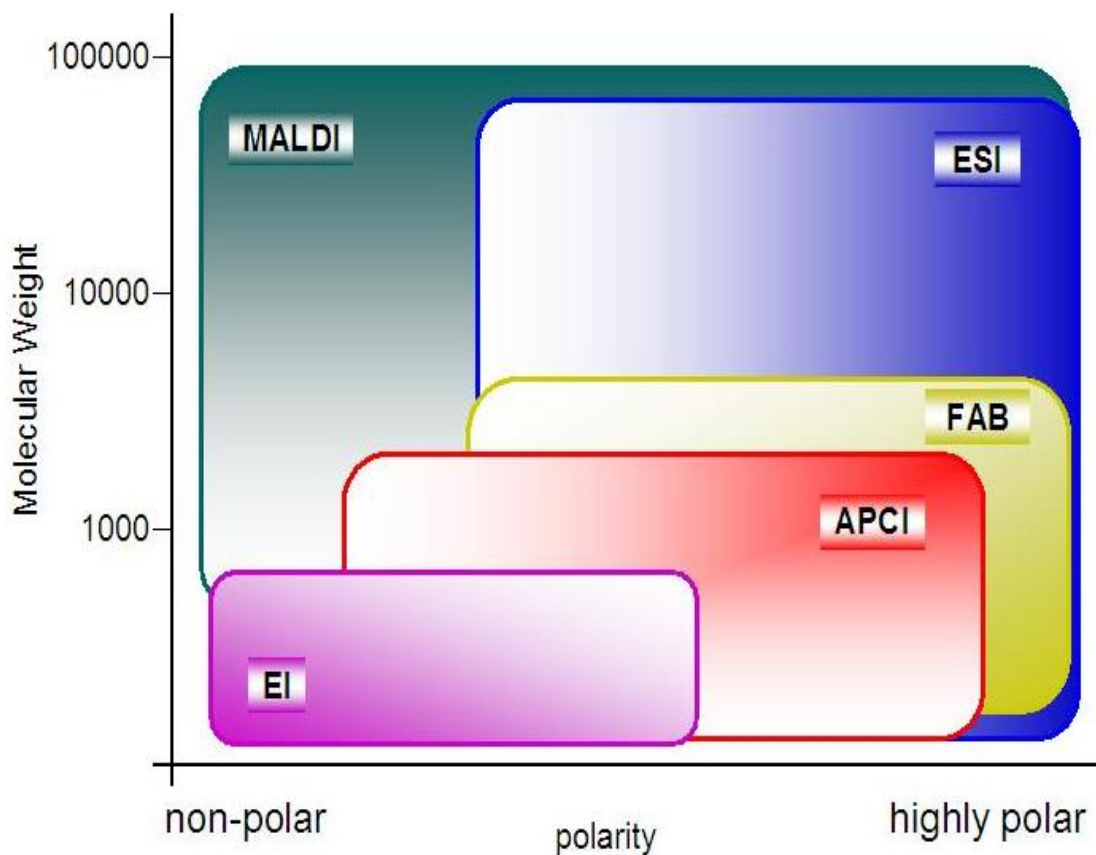



# DETECTOR

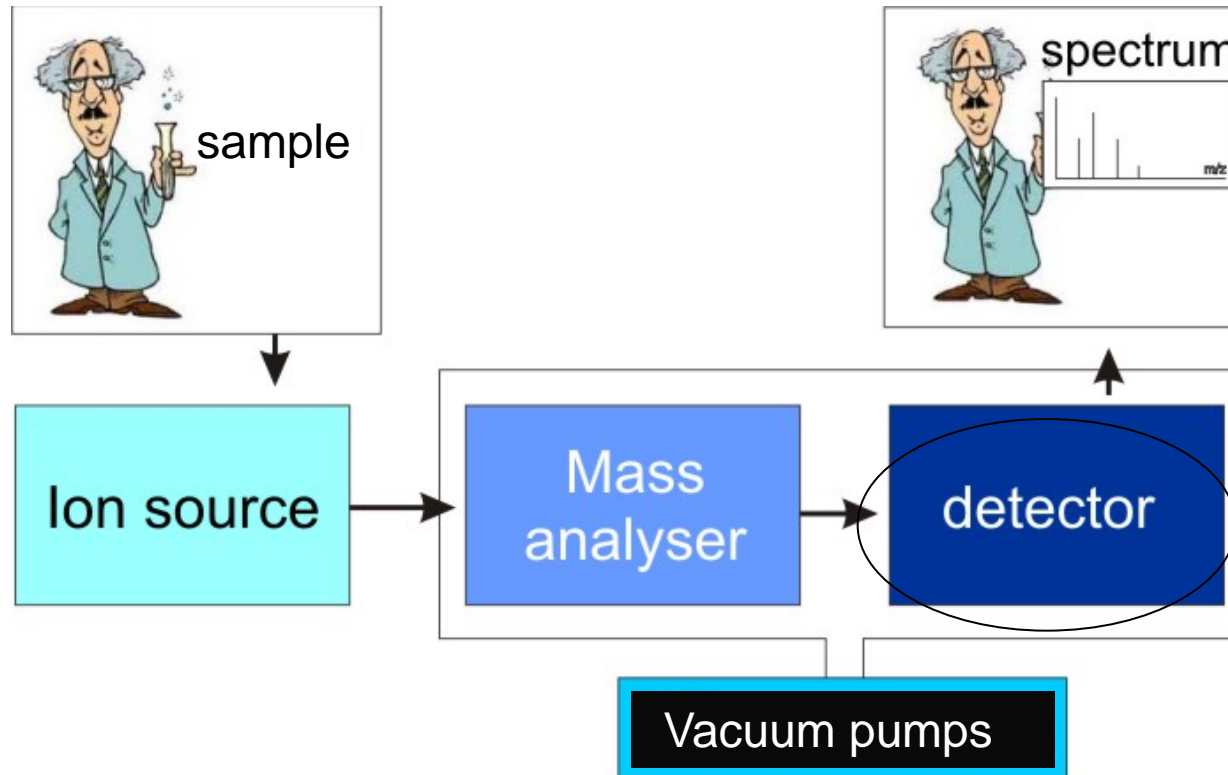

- Detectors - record the charge induced or the current produced, when an ion passes by or hits a surface







# DETECTORS

- Records the current produced, when an ion hits a surface.
- In commercial instrument detectors with conversion dynode
  - Ions strike a conversion dynode to produce electrons – electron multiplied by
    - Electron multiplier
    - Ion-to-photon detector
- Record the charge induced, when an ion passes by
  - FT-ICR-MS and Orbitrap
    - The detector is part of analyser
    - Ions only pass near the electrodes




# DETECTORS

- Elektromultiplier with discrete dynodes
  - Amplification  $10^6$
- Chaneltron
  - PbO - sensitive surface
  - Amplification  $10^6$
- Microchannel Plate Detectors (MCP)
  - PbO - sensitive service
  - Amplification  $10^3$ 
    - Two detectors –  $10^6$
  - For TOF analyser
- Ion-to-photon detector
  - Electron strike a phosphor and the resulting photons are detected by a photomultiplier

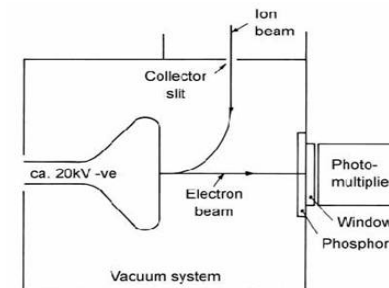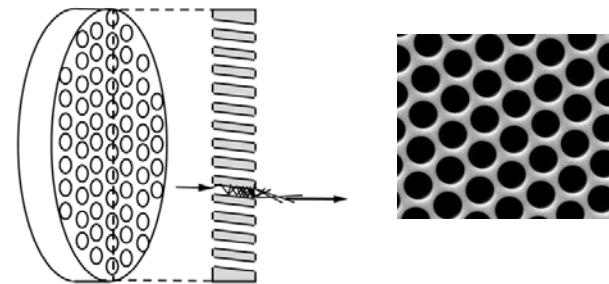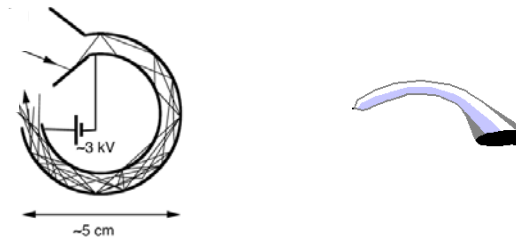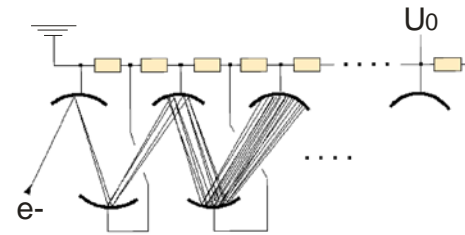

# VACUUM SYSTEM

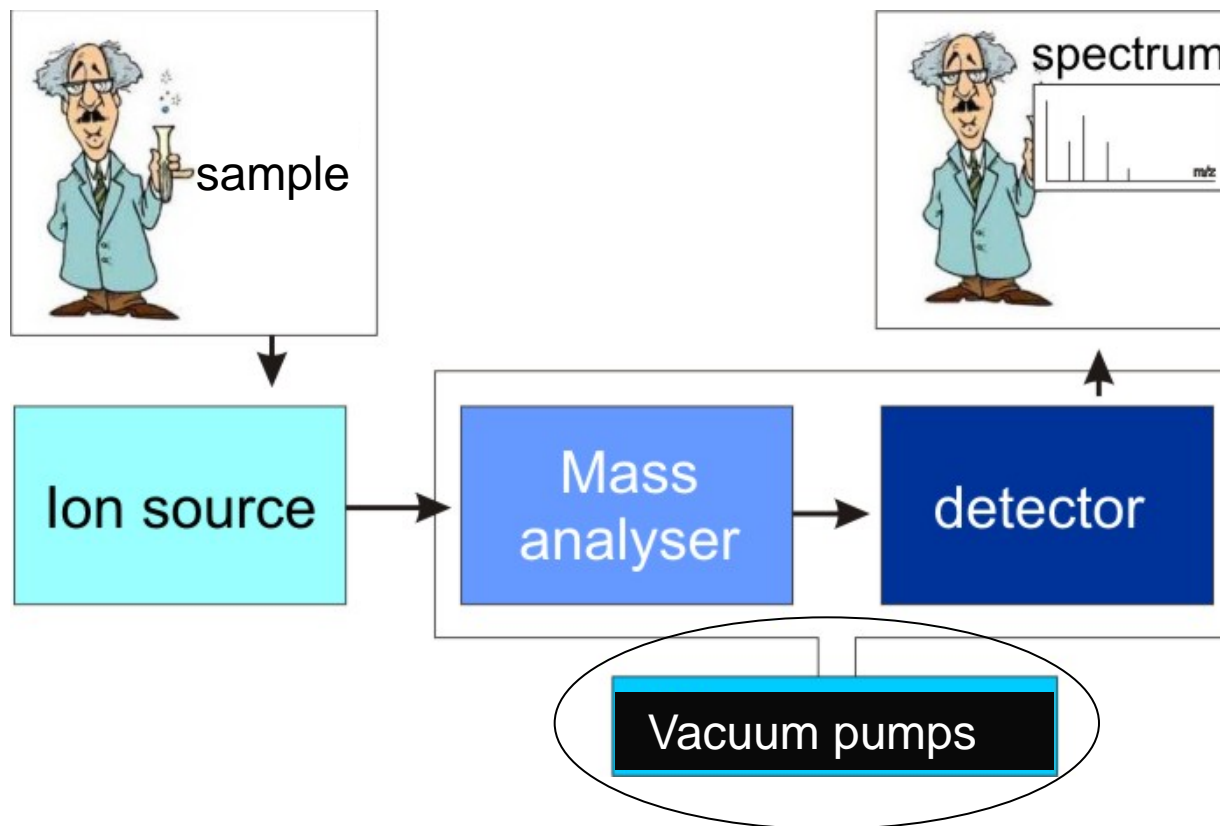

# VACUUM SYSTEMS

- Usually two steps
  - Rough vacuum (roughing pump - membrane pump, oil-sealed roughing pump, scroll pump)
    - 100 – 0.1 Pa
    - all type of instruments
  - High vacuum (**turbomolecular pump**, diffusion pump)
    - $0.1 \cdot 10^{-6}$  Pa,
    - TOF, Q, IT
- Ultra-high vacuum (turbomolecular pump)
  - ( $10^{-10}$ - $10^{-12}$  Pa)
  - Orbitrap, ICR



THANK YOU FOR YOUR ATTENTION

