

The Influence of Purification of Carp Collagen Used in a Novel Composite Graft with Sandwich Construction of the Wall on Its Biological Properties and Graft Patency Rates

P. MITAS^{1*}, T. GRUS^{1*}, L. LAMBERT², M. MLCEK³, H. CHLUP⁴, E. HONSOVA⁵,
M. DOHNALOVA¹, T. SUCHY⁶, A. BURGETOVA², J. LINDNER¹, M. SPACEK¹

*These authors contributed equally to this paper

¹Second Department of Surgery - Department of Cardiovascular Surgery, First Faculty of Medicine, Charles University and General University Hospital, Prague, Czech Republic, ²Department of Radiology, First Faculty of Medicine, Charles University and General University Hospital in Prague, Prague, Czech Republic, ³Institute of Physiology, First Faculty of Medicine, Charles University, Prague, Czech Republic, ⁴Department of Mechanics, Biomechanics and Mechatronics, Faculty of Mechanical Engineering, Czech Technical University in Prague, Prague, Czech Republic, ⁵Department Pathology, Institute for Clinical and Experimental Medicine, Prague, Czech Republic, ⁶Institute of Rock Structure and Mechanics of the Czech Academy of Sciences, Prague, Czech Republic.

Received January 12, 2019

Accepted May 2, 2019

Epub Ahead of Print June 6, 2019

Summary

We compared graft outcome between two types of a novel composite three-layer carp-collagen-coated vascular graft in low-flow conditions in a sheep model. Collagen in group A underwent more cycles of purification than in group B in order to increase the ratio between collagen and residual fat. The grafts were implanted end-to-side in both carotid arteries in sheep (14 grafts in 7 sheep in group A, 18 grafts in 9 sheep in group B) and artificially stenosed on the right side. The flow in the grafts in group A decreased from 297 ± 118 ml/min to 158 ± 159 ml/min ($p=0.041$) after placement of the artificial stenosis in group A, and from 330 ± 164 ml/min to 97 ± 29 ml/min ($p=0.0052$) in group B ($p=0.27$ between the groups). From the five surviving animals in group A, both grafts occluded in one animal 3 and 14 days after implantation. In group B, from the six surviving animals, only one graft on the left side remained patent ($p=0.0017$). Histology showed degradation of the intimal layer in the center with endothelialization from the periphery in group A and formation of thick fibrous intimal layer in group B. We conclude that the ratio between collagen and lipid content in the novel three-layer graft plays a critical role in its patency and structural changes *in vivo*.

Key words

Vascular graft • Collagen • Crosslinking • Extrusion • Composite tube • Patency • Sheep

Corresponding author

L. Lambert, Department of Radiology, First Faculty of Medicine, Charles University and General University Hospital in Prague, U Nemocnice 2, 128 08 Prague 2, Czech Republic. Fax: +420 224963048. E-mail: lambert.lukas@gmail.com

Introduction

The long-term patency of prosthetic vascular grafts in the treatment of peripheral arterial disease depends on numerous factors including morphology of the anastomosis, graft diameter, and the outflow bed. In distal reconstructions and reconstructions with limited outflow, prosthetic grafts show worse patency rates than in proximal reconstructions (Chlupáč *et al.* 2009, Grus *et al.* 2017).

Our group has designed and manufactured a novel composite three-layer vascular graft. It is a composite tube on a biological basis with sandwich

construction of the wall where a polyester mesh is covered on both sides by collagen prepared from freshwater fish (Browning *et al.* 2012, McClure *et al.* 2012, Yamada *et al.* 2014). Previously, the immunological properties of carp collagen were tested and found comparable to or even better than the commonly used bovine collagen (Duan *et al.* 2009, Lambert *et al.* 2019, Yamamoto *et al.* 2014). We and other research groups tested different designs of vascular grafts with regard to similarity with a native vessel (Singh *et al.* 2015, Spacek *et al.* 2019, Veselý *et al.* 2015, Wise *et al.* 2011).

Preparation of collagen from a biological material follows numerous steps that include harvesting, cleaning, grinding, homogenization, crosslinking, and sterilization. Each of these steps influences properties of the final product. Specifically, crosslinking decreases compliance and thrombogenicity of the material (Terzi *et al.* 2018). The effect of the proportion of collagen and residual fat content which is influenced by its repeated dissolution and washing has not been explored yet.

In the present study, we manipulated the residual fat content in collagen used in this graft to influence its patency and biological properties that we further tested in an animal model.

Materials and Methods

This prospective study was approved by the institutional Animal Care and Use Committee and conducted in accordance with national Act No 246/1992 Coll. as amended on the protection of animals against cruelty, that is harmonized with the legislation of EU.

Two types of a composite three-layer vascular graft for low flow conditions with two carp collagen layers covering polyester mesh from both sides with an internal diameter of 5 mm were prepared (Grus *et al.* 2018, Spacek *et al.* 2019). The middle layer (Fig. 1) was knitted from a polyester monofilament (TDA Inc., Connecticut, USA) with a diameter of 34 µm prepared by electrospinning on a flat double knitting machine (Faculty of Textile Engineering, Technical University in Liberec, Czech Republic) with 16 needles, 32 loops and then soaked in a solution with 4 g/l AEL (nonionic tenside), 0.5 g/l Na₂CO₃ at 80 °C for one hour, washed in chloroform for one hour, and finally thermally fixed at 160 °C for 10 min (Grus *et al.* 2018, Spacek *et al.* 2019). Mechanical and immunological properties of this graft have been tested previously (Lambert *et al.* 2019, Spacek *et al.* 2019).

Collagen was extracted from the skin of young (≤ 2 kg) scaleless carps. The skin was cleaned, frozen, and minced. This material was repeatedly dissolved in 0.1 M NaOH to remove excessive fat, washed, and again repeatedly dissolved in 10 % n-butanol, filtered and washed. The number of dissolution cycles in NaOH was 5 in product A and 3 in product B. Ultimately, collagen sheets were prepared by crosslinking in formaldehyde for 8 minutes (2.2 % Lyofix CHN) and curing in 20 % glycerine for 30 min. In the final product, we estimated the content of dry matter, collagen, and fat, and measured the heat-shrink temperature. The middle layer was coated by collagen from both sides by extrusion creating a three-layer graft. The final product with an internal diameter of 5 mm was sterilized by gamma irradiation.

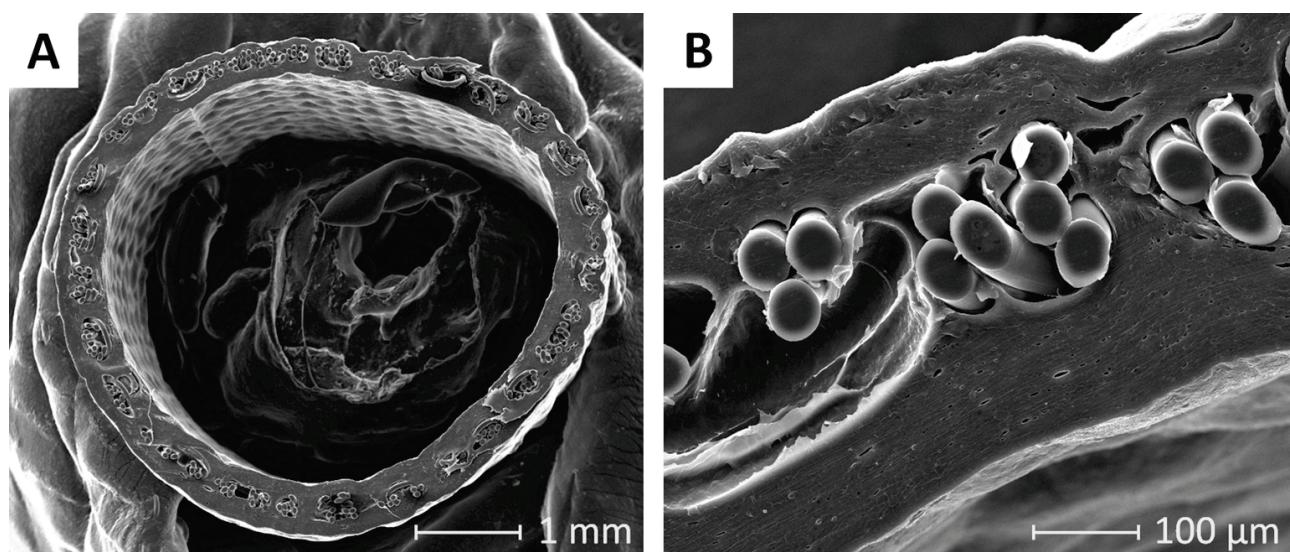


Fig. 1. MicroCT image of the novel three-layer graft.



Fig. 2. Photograph of the graft ($\varnothing = 5$ mm) before (above) and after (below) implantation. Proximal and distal end of the anastomosis are marked with arrowheads. Arrow shows the direction of blood flow. Asterisk marks the plastic band used for artificial narrowing. The perivascular transient-time ultrasonic probe is marked by a chevron.

Table 1. Composition of collagen product A and B used in the inner and outer layer of the graft.

	Product A (lower fat content)	Product B (higher fat content)
Dry matter	7 %	8 %
Collagen in dry matter	81 %	57 %
Fat in dry matter	6 %	34 %

The grafts were trimmed to a length of approx. 15 cm and implanted end-to-side in both carotid arteries in a sheep by two experienced vascular surgeons during general inhalation anesthesia (Fig. 2). There were 14 grafts coated with product A implanted in 7 sheep (group A) and 18 grafts coated with product B implanted in 9 sheep (group B). The sheep were 6.3 ± 1.0 years old, weighted 53 ± 14 kg, and 12 (75 %) were ewes. Flow in the carotid artery and graft were measured using a perivascular transient-time ultrasonic probe (Transonic Inc., Ithaca, NY) before and after implantation. In all animals, the outflow artery was artificially narrowed by placing a plastic band on one side (Fig. 2) to limit the flow to 100–150 ml/min, and the flow was re-measured. Postoperatively, all animals were receiving acetylsalicylic acid (Anopyrin 100 mg, Zentiva, Czech Republic). The patency of the grafts was assessed by ultrasound (Acuson

X150™, Siemens Healthcare, Munich, Germany) and the general status of the animals was checked on a regular basis. The animals were terminated when 1) they were not thriving or could not recover from anesthesia, 2) the graft occluded, or 3) after a period of 26 weeks. The grafts were explanted for histological analysis. The specimens were processed with the paraffin technique and stained with hematoxylin and eosin (H&E) with Weigert's resorcin-fuchsin (elastin).

Results

Product A had higher content of collagen and lower content of fat compared to product B (Table 1). The heat-shrink temperature in product A and B was comparable with 43.1 °C and 43.7 °C, respectively. When handling, product B with higher fat content was more

compliant with better cohesion of the layers while product A was tougher, more brittle, with suboptimal cohesion of the layers.

In each group, two animals did not fully recover from the anesthesia. One animal in group A and one animal in group B were terminated at 51 and 5 days for failure to thrive. In group A, two grafts in one animal occluded in the first two weeks, but in group B, early closure was observed in five animals (Fig. 3). The flow through the graft was comparable between the study groups and the left and right side (Table 2). After artificial narrowing, the flow in the graft diminished by 47 % in group A and by 71 % in group B, but the difference between the groups was not significant ($p=0.28$). Histological analysis showed that grafts that were *in situ* for at least three weeks induced cellular reaction in the outer layer. Grafts from group A showed

areas of exposed polyester mesh in the central portion with signs of patchy to sub-confluent endothelialization towards the periphery (Fig. 4). Graft from group B developed a thick fibrous intimal layer (Fig. 5).

Discussion

This study showed that the use of carp collagen with lower fat content (product A) in a novel composite three-layer graft with sandwich construction of the wall results in better patency rates. Both collagens showed tendency to incorporate in the surrounding tissue. Grafts coated with higher carp collagen content (product A) show degradation of the intimal layer and reendothelialization from the periphery while grafts with higher lipid content (product B) tend to develop a thick fibrous intimal layer.

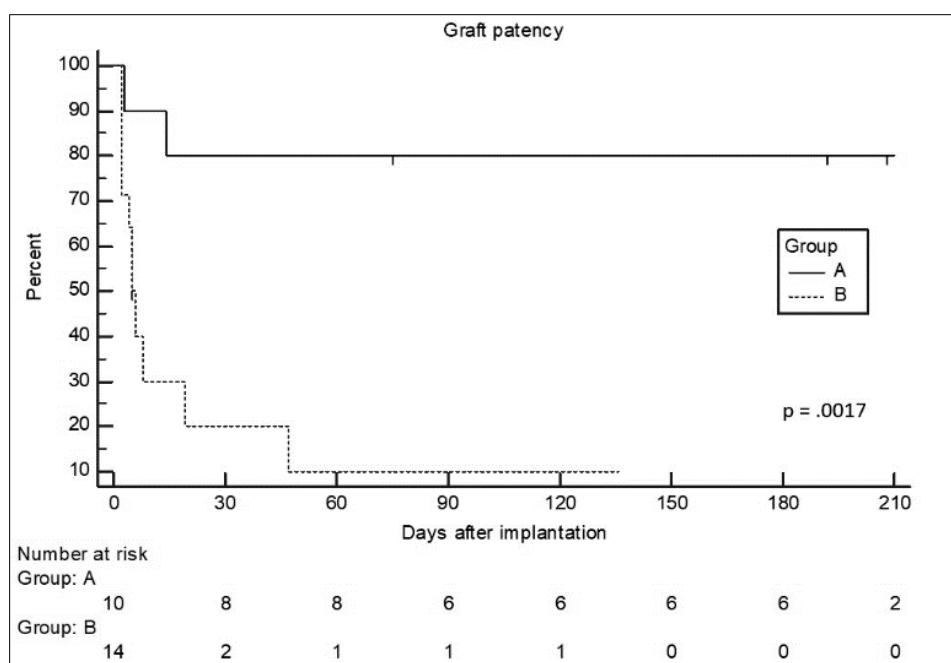


Fig. 3. Kaplan-Meier plot of graft patency rates shows clear difference between group A (lower fat content collagen) and group B (higher fat content collagen) with $p=0.0031$ according to the log-rank test.

Table 2. Flow rates before and after implantation of the graft, after artificial narrowing of the right side to limit flow through the graft, and at the end of the experiment in animals with patent grafts. The graft implanted in group A was coated with collagen with lower fat content (product A) compared to the graft used in group B (see Table 1).

Group	Side	Flow after graft placement		Flow after narrowing		Flow at the end	
		Flow Initial [ml/min]	[ml/min]	p^1	[ml/min]	p^1	[ml/min]
A	Left	350±120	287±113	0.1434		355±102	0.42
A	Right	309±134	297±118	0.7645	158±159	0.0411	147±10
B	Left	330±170	311±123	0.5674		175	x
B	Right	318±137	330±164	0.7719	97±29	0.0052	110

¹paired t-test

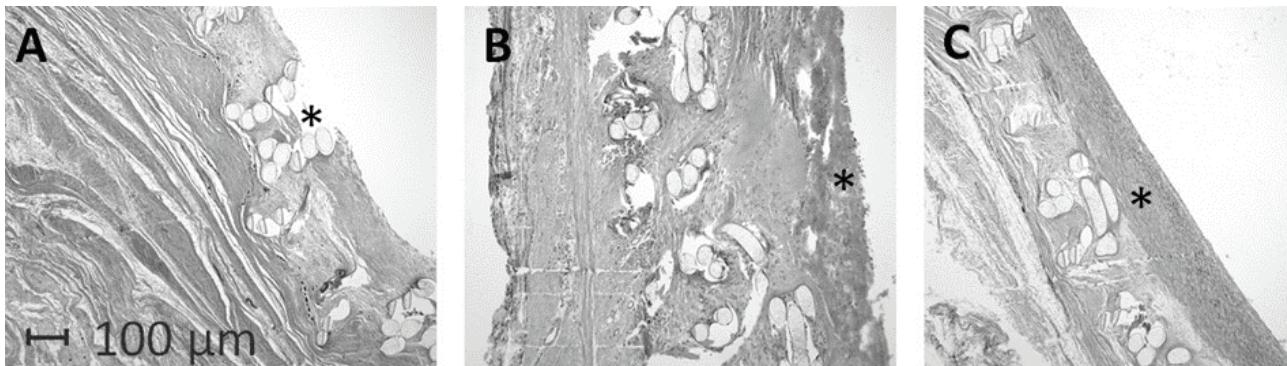


Fig. 4: Microscopic image (H&E) of an explanted graft shows: a) areas of exposed polyester mesh in the center, b) intimal hyperplasia, and c) mild fibrous thickening of the intimal layer towards the periphery of the graft indicating neoendothelisation in an animal from group A (lower fat content collagen), all marked by an asterisk.

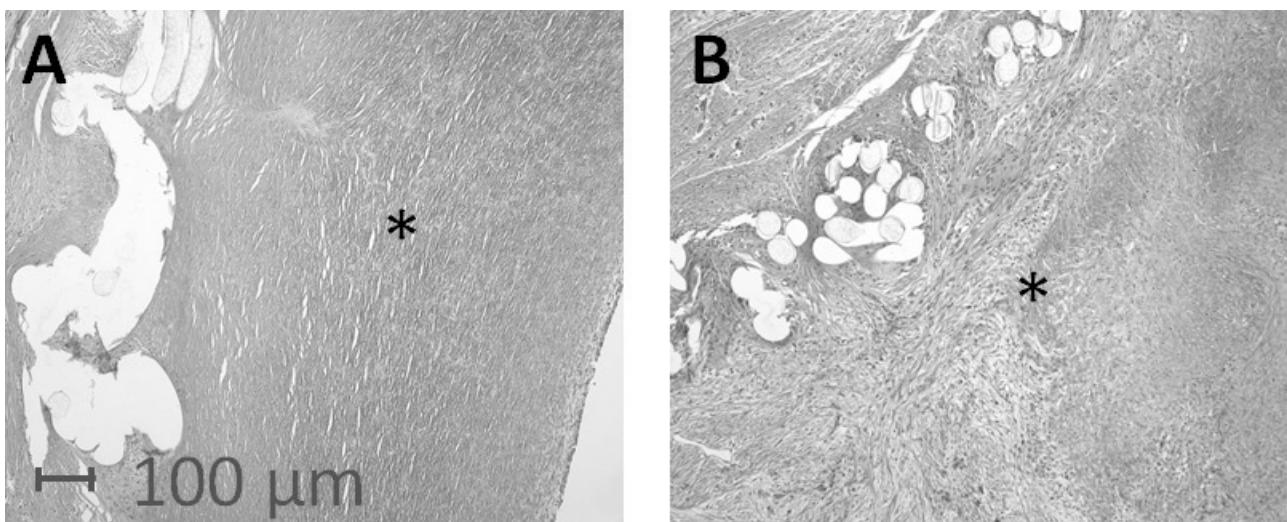


Fig. 5. Microscopic image (H&E) of an explanted graft shows marked fibrous thickening of the intimal layer in two animals from group B (higher fat content collagen), marked by an asterisk.

Prosthetic vascular grafts are an alternative to autologous grafts if they are not available in sufficient length or quality. Generally, their long-term performance is inferior to autologous grafts, but some studies have shown, that it may be even comparable in proximal reconstructions (Rychlik *et al.* 2014). In our design of a three-layer vascular graft, we aimed to mimic the structure of an autologous vessel and approximate its mechanical and physical properties as much as possible (Spacek *et al.* 2019, Veselý *et al.* 2015). For this, we tested various constructions of the vessel wall and structures of the scaffold in previous studies (Grus *et al.* 2018, Spacek *et al.* 2019).

The fabric and construction of a prosthetic vascular graft has an effect on its long-term patency as well (Sarkar *et al.* 2007). Currently, two types of grafts are in clinical use: the expanded polytetrafluoroethylene (ePTFE) graft, and knitted grafts made from polyester

with several modifications of the graft structure and inner wall coating. Several graft construction types including bi- or multi-layered design have been proposed and investigated even by our research group (Chlupáč *et al.* 2009, Spacek *et al.* 2019). Coating of the inner layer by a modified mesh to improve wettability and neoendothelialization of the graft have been proposed and tested in animal models but were not used in patients (Grus *et al.* 2018). In this study, we showed, that modification of a single step in purification of the collagen impacts the balance between degradation of the artificial intima, neoendothelialization, and proliferation and hypertrophy of this layer. The primary idea of modifying the ratio between the collagen content and residual fat was to decrease wettability of the inner layer because pure collagen is a hemostatic agent.

As Zilla *et al.* (Zilla *et al.* 2007) indicated, the ingrowth of the intima from the native vessel to the

periphery of the graft is not as desirable as transmural reendothelialization along the whole length of the graft. In group A (lower fat content in collagen), we observed the first pattern. In group B, we believe that the latter phenomenon prevailed, but it was too intense that it resulted in stenosis and ultimately occlusion of the vessel. The residual fat content in the collagen layer, which was higher in group B, may dissolve from the mesh, which results in rarefaction of the inner layer, increased porosity, and throughput. We assume that accelerated release of the fat from the inner layer in group B resulted in increased porosity and exposure of collagen fibers and thus increased adhesion of fibrin and platelets forming a thick neointimal fibrinous layer.

Mechanical properties of a vascular graft in terms of handling and constructing an anastomosis are important. We noted that product B with higher fat content was easier to handle due to its better compliance and cohesion of the layers, but this also resulted in greater tortuosity and propensity to kinking. Product A with lower fat content was more difficult to suture, and attention had to be paid not to dissociate its layers, but its shape was more stable.

Extracted carp collagen has a heat-shrink temperature about 20 °C which increases with cross-linking, in our study to 43 °C. Normal body temperature of a sheep is 39 °C which is close to this temperature and this also may have had impact on the stability of the collagen layer, its wettability, thrombogenicity, porosity, and throughput, which should not exceed 3.000 ml/min/cm²/120 mmHg. Further design of the graft therefore would need to address this issue by longer time for cross-linking (Vesely *et al.* 2015). It should be noted that sterilization by gamma rays increases the crosslinking rate (Matuska and McFetridge 2015). Crosslinking increases stiffness of the material and has another side effect of changing the epitopes of the collagen macromolecule that are responsible for its hemostatic properties and therefore may contribute to decreased thrombogenicity (Chan and Leong 2008, Terzi *et al.* 2018, Wise *et al.* 2011). Also, formaldehyde should be replaced by a different non-carcinogenic crosslinking agent, when used in humans.

The outer layer plays a role in incorporation of the graft into the surrounding structures. In our study, the

manipulated properties of the collagen showed little influence on cellular migration into the outer artificial collagen layer.

Apart from graft type, there are several factors known to influence long term patency of the reconstruction. Previously, our group and others have demonstrated the favorable effect of constructing an anastomosis with an acute angle, or the choice of the graft diameter similar or slightly greater than the target artery (Grus *et al.* 2009, Grus *et al.* 2016a, Grus *et al.* 2016b). In our experiment, we constructed a graft with a diameter of 5mm, which is similar to that of the carotid artery in a sheep. However, experimental manipulation of the flow could have tipped the balance towards lower wall shear stress and increased thrombogenicity (Zhou *et al.* 2014). On the other hand, increased wall shear stress may accelerate degradation of the inner layer and impede formation of the neointima. The anastomosis undergoes remodeling that promotes laminar flow in the first postoperative months as well (Grusova *et al.* 2018).

This study has several limitations. Firstly, the number of surviving animals especially in group B (higher fat content) was small. Secondly, the flow on the artificially stenosed side in group B was slightly, albeit not significantly, smaller. Thirdly, the experiment was carried out on an animal model and its results cannot be fully translated to human patients. Further study with longer follow-up is warranted to assess graft patency in long-term.

Conclusions

This study showed that modification of the fat content of collagen used in the outer and inner layer of a novel composite three-layer vascular graft plays a critical role in its patency and structural changes in the intimal layer.

Conflict of Interest

There is no conflict of interest.

Acknowledgements

This work was supported by Ministry of Health of the Czech Republic (grant 15-27941A) and by the grant SVV-2019 - 260 372.

References

- BROWNING MB, DEMPSEY D, GUIZA V, BECERRA S, RIVERA J, RUSSELL B, HÖÖK M, CLUBB F, MILLER M, FOSSUM T, DONG JF, BERGERON AL, HAHN M, COSGRIFF-HERNANDEZ E: Multilayer vascular grafts based on collagen-mimetic proteins. *Acta Biomater* **8**: 1010-1021, 2012.
- CHAN BP, LEONG KW: Scaffolding in tissue engineering: general approaches and tissue-specific considerations. *Eur Spine J* **17**: 467-479, 2008.
- CHLUPÁČ J, FILOVÁ E, BACÁKOVÁ L: Blood vessel replacement: 50 years of development and tissue engineering paradigms in vascular surgery. *Physiol Res* **58** Suppl 2: S119-139, 2009.
- DUAN R, ZHANG J, DU X, YAO X, KONNO K: Properties of collagen from skin, scale and bone of carp (*Cyprinus carpio*). *Food Chem* **112**: 702-706, 2009.
- GRUS T, GRUSOVA G, LAMBERT L, BANERJEE R, MATECHA J, MLCEK M: The influence of the anastomosis angle on the hemodynamics in the distal anastomosis in the infrainguinal bypass: an *in vitro* study. *Physiol Res* **65**: 591-595, 2016a.
- GRUS T, LAMBERT L, GRUSOVA G, LUKAC P, HRUBY J, LINDNER J: Branched crural bypass has no advantage over simple crural bypass in the treatment of peripheral arterial disease. *Int J Clin Exp Med* **10**: 7859-7866, 2017.
- GRUS T, LAMBERT L, MATĚCHA J, GRUSOVÁ G, ŠPAČEK M, MLČEK M: The ratio of diameters between the target artery and the bypass modifies hemodynamic parameters related to intimal hyperplasia in the distal end-to-side anastomosis. *Physiol Res* **65**: 901-908, 2016b.
- GRUS T, LAMBERT L, MLCEK M, CHLUP H, HONSOVA E, SPACEK M, BURGETOVA A, LINDNER J: *In vivo* evaluation of short-term performance of new three-layer collagen-based vascular graft designed for low-flow peripheral vascular reconstructions. *Biomed Res Int* **2018**: 3519596, 2018.
- GRUS T, LINDNER J, VIDIM T, TOSOVSKY J, MATECHA J, ROHN V, LAMBERT L, GRUSOVA G: The anastomosis angle is a key to improved long-term patency of proximal femoropopliteal bypass. *Ann Vasc Surg* **23**: 598-605, 2009.
- GRUSOVA G, LAMBERT L, KAVAN J, LAMBERTOVA A, BURGETOVA A, MLCEK M, GRUS T: Natural remodeling of the distal anastomosis of an above-knee femoropopliteal bypass depicted by CT angiography of lower limbs improves geometry of the reconstruction. *Physiol Res* **67**: 857-862, 2018.
- LAMBERT L, NOVAKOVA M, LUKAC P, CECHOVA D, SUKENIKOVA L, HRDY J, MLCEK M, CHLUP H, SUCHÝ T, GRUS T: Evaluation of the immunogenicity of a vascular graft covered with collagen derived from the european carp (*cyprinus carpio*) and bovine collagen. *Biomed Res Int* **2019**: 5301405, 2019.
- MATUSKA AM, MCFETRIDGE PS: The effect of terminal sterilization on structural and biophysical properties of a decellularized collagen-based scaffold; implications for stem cell adhesion. *J Biomed Mater Res B Appl Biomater* **103**: 397-406, 2015.
- MCCLURE MJ, SIMPSON DG, BOWLIN GL: Tri-layered vascular grafts composed of polycaprolactone, elastin, collagen, and silk: Optimization of graft properties. *J Mech Behav Biomed Mater* **10**: 48-61, 2012.
- RYCHLIK IJ, DAVEY P, MURPHY J, O'DONNELL ME: A meta-analysis to compare Dacron versus polytetrafluoroethylene grafts for above-knee femoropopliteal artery bypass. *J Vasc Surg* **60**: 506-515, 2014.
- SARKAR S, SCHMITZ-RIXEN T, HAMILTON G, SEIFALIAN AM: Achieving the ideal properties for vascular bypass grafts using a tissue engineered approach: a review. *Med Biol Eng Comput* **45**: 327-336, 2007.
- SINGH C, WONG CS, WANG X: Medical textiles as vascular implants and their success to mimic natural arteries. *J Funct Biomater* **6**: 500-525, 2015.
- SPACEK M, CHLUP H, MITAS P, VESELY J, LAMBERT L, MLCEK M, KRAJICEK M, LINDNER J, GRUS T: Three-layer collagen-based vascular graft designed for low-flow peripheral vascular reconstructions. *J Appl Biomed* **17**: 47-52, 2019.
- TERZI A, STORELLI E, BETTINI S, SIBILLANO T, ALTAMURA D, SALVATORE L, MADAGHIELE M, ROMANO A, SILIQI D, LADISA M, DE CARO L, QUATTRINI A, VALLI L, SANNINO A, GIANNINI C: Effects of processing on structural, mechanical and biological properties of collagen-based substrates for regenerative medicine. *Sci Rep* **8**: 1429, 2018.

- VESELÝ J, HORNÝ L, CHLUP H, ADAMEK T, KRAJÍČEK M, ŽITNÝ R: Constitutive modeling of human saphenous veins at overloading pressures. *J Mech Behav Biomed Mater* **45**: 101-108, 2015.
- VESELY J, HORNÝ L, CHLUP H, BERAN M, KRAJICEK M, ŽITNÝ R: Effect of polyvinyl alcohol concentration on the mechanical properties of collagen/polyvinyl alcohol blends. *Appl Mech Mater* **732**: 161-164, 2015.
- WISE SG, BYROM MJ, WATERHOUSE A, BANNON PG, NG MKC, WEISS AS: A multilayered synthetic human elastin/polycaprolactone hybrid vascular graft with tailored mechanical properties. *Acta Biomater* **7**: 295-303, 2011.
- YAMADA S, YAMAMOTO K, IKEDA T, YANAGIGUCHI K, HAYASHI Y: Potency of fish collagen as a scaffold for regenerative medicine. *Biomed Res Int* **2014**: 302932, 2014, doi: 10.1155/2014/302932
- YAMAMOTO K, IGAWA K, SUGIMOTO K, YOSHIZAWA Y, YANAGIGUCHI K, IKEDA T, YAMADA S, HAYASHI Y: Biological safety of fish (tilapia) collagen. *Biomed Res Int* **2014**: 630757, 2014. doi: 10.1155/2014/630757
- ZHOU J, LI Y-S, CHIEN S: Shear stress-initiated signaling and its regulation of endothelial function. *Arterioscler Thromb Vasc Biol* **34**: 2191-2198, 2014.
- ZILLA P, BEZUIDENHOUT D, HUMAN P: Prosthetic vascular grafts: Wrong models, wrong questions and no healing. *Biomaterials* **28**: 5009-5027, 2007.